



STS Instruments - Siloxane Monitor Specification

The STS Siloxane Monitor is CE certified and complies with IGE SR25 requirements.

The Siloxane monitor has the following requirements:

1. 110V 6A – (IEC rear connector) wired to flex outlet from Distribution box.
2. N2 carrier gas line: ¼" Nylon/PTFE/SS piping (1/4" Swagelok connector supplied) Set at 1Bar at cylinder regulator Technical Grade 99.999%.
3. Biogas feed line - ¼" PTFE/SS piping (1/4" Swagelok connector supplied) Maximum 1Bar input pressure.
4. Vent line - ¼" PTFE/SS piping (1/4" Swagelok connector supplied) Vented ~2m above head height (U bend to prevent water ingress) , end of Line flame arrester to be fitted.

The water Traps require the following:

1. 24V supplied from instrument via Ancillary Box for auto drain (WT)
2. Water Drain line - ¼" PTFE piping (Push fit connector)
3. Water Vented external to kiosk at ground level.
4. Biogas Gas connections – The water trap (WT) uses a 1/4" Swagelok connection. The Coalescing filter is a ¼" Swagelok & the Flame arrester is a ¼" Swagelok.

The heated Line requires the following:

1. 110V 16A – Directly wired from distribution box.
2. Temperature set to 60degC.
3. Cut to length - Requires sealing at cut end.

Biogas Flow rates:

The instrument samples approx. 2L of biogas during a 20minute window every 1hour, at a flow of approx. 100ml/min. This is passed through the instrument then vented to atmosphere.

N2 Flow rate:

The instrument consumes approx. 4L of N2 every hour. Resulting in 0.1m³ of N2 per day. This is passed through the instrument then vented to atmosphere.

STS recommend using the largest N2 cylinder to avoid regular replacement.

Air Products: X47S: 80kg 200bar 8.9m³. Technical Grade.

Regulator : BOC 8500 or similar, 300Bar inlet , 0-4 bar outlet.

This should last approx. 90days, 3 months.

Kiosk requirements:

A GRP kiosk is required as per the manual specification.



STS Instruments Ltd

The kiosk will require 6 external connections:

1. Biogas IN
2. N2 IN
3. Vent OUT
4. Drain OUT
5. Heated Line out
6. Heated Line Sensor out.

Biogas Supply:

Regulated in the kiosk to 35mbar, normal inlet pressure to the regulators should not exceed 350mbar. If a higher pressure is present, the regulator will require re-specification.

The electrical supply:


A 110V connection is required to the externally mounted switch. This is routed to a Distribution box in the kiosk where there are a 6A RCD to the instrument, and a 16A RCD directly wired to the heated line. All earthed. (it may be necessary to additionally fit a cabinet heater which is specified at 400w 110V peak current 9A)

Safety:

1. The instrument uses an air purge system to ensure safe operation, this is achieved with 2 high capacity fans mounted in the instrument which force a constant stream of air through the case. The instrument fans are connected to vent plates in the kiosk by flexible hoses. The flow of air through the instrument ensures that even in a catastrophic joint failure that the LEL of CH₄ would not be exceeded. The purge fans are monitored so that if they are inactive the instrument will be placed into "Safe Mode"
2. The instrument has an on-board methane sensor which will place the instrument into "Safe Mode" if it exceeds 10% of the LEL. An on-board temperature sensor will place the instrument in "Safe Mode" if the temperature in the cabinet exceeds 50C.
3. Incoming bio-gas lines are controlled by Solenoid valves which are in the Normally Closed position unless activated, the instrument also has a solenoid valve on the incoming biogas line which is Normally Closed, any power failure will therefore close these valves stopping gas flow. "Safe mode" shuts the incoming gas valves, turns off all heaters and runs the case fans to vent.
4. The kiosk itself is cross ventilated from a further two ventilation grilles.

The Siloxane Monitor & Kiosk is not EX or Atex rated and as such should be sited outside of any zoned area.

Electrical Circuit

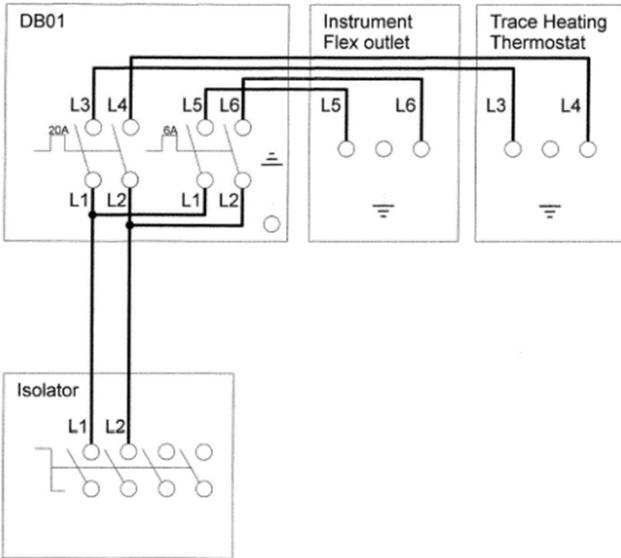

Instrument Kiosk Layout



STS Instruments Ltd

FRONT

